
STEADLIVE 思泰利
MEDICAL APPARATUS & HEALTHY NURSING

# Colostomy bag instruction

Two System

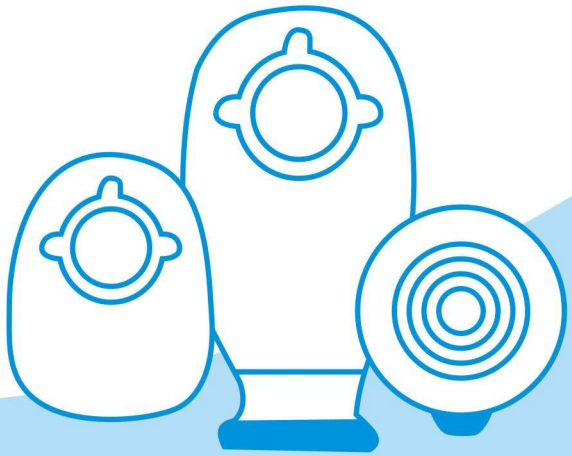

## Two System Colostomy Bag

1. Use the water to clean the skin around stoma.

2. A hole have been advanced open at the, flange the sufferers can cut a hole at the flange at the basis of the kind of stoma.



3. Remove the protection paper at the flange.



4. Put the flange which have been cut well aimed at the stoma and stick on unclitly, press it down lightly by using the finger, make the flange stick on well. Notice: the two microtias which include the hole and the sash at the parallel direction.



5. Blow little air into the bag before fixing the bag in order to prevent the wall of the pocket being sticked on . then hold the cutting sleeve aimed at the wedge seat using the two hands, from the bottom, the finger press it carefully along the cutting sleeve, make wedge seat and the cutting sleeve solid absolutely.



6. When have to change the bag put one finger to press on flange, another finger to press the middle, little protruding of the cutting sleeve and pult forth, unbolt the bag.



7. Use one finger to press the skin, another finger to tear out flange carefully when have to change the flange.



8. Use clip to clamp the end of bag, agraffe type must be press the end of bag and turn forth 2 circum ference then join the agraffe before use the drainable bag.



9. Open the end of the bag when giving out stool, make the end of the bag aim at the urinal, and then wash the end of the bag as the picture, make the end of the bag smoothly, then can reuse.




## Notice

1. The sufferer of the intestines open can use this product to incept the ordure only.

2. The "flange" to mix this product can use 3-5days in normal condition, it can affect the effect of the affixing if use delay, it is not good to the skin .

3. If the bag full of air, make it exhausted by using the pinhole in the upper end of the bag. suggest use activated carbon cassette, it can wipe off the peculiar smell.

4. The chassis and the bag which being exchanged can not be used againg.



5. The flange and the bag which can not be washed into the toilet or cloaca, it can not be discarded at will, pay attention to the protection of the environment.




6. The skin uses to the gum allergy carefully.

Wuhan Sitaili Medical Apparatus Development Co., Ltd.
Room1-8,7th Floor,7th Building Guannan Fuxing Medical Industrial Park,No.62 Guanggu Road, East Lake New Technology Development Zone Wuhan City, Hubei Province, China, Tel: +86-27-82302765
EC Representative: Prolinx Gmbh
Address: Brehmstr.56,40239, Duesseldorf, Germany, Tel: 0049 211 3105 4698

STEADLIVE 思泰利
MEDICAL APPARATUS & HEALTHY NURSING

# Οδηγίες χρήσηςσάκων στομίας

## Σάκος δύο τεμαχίων

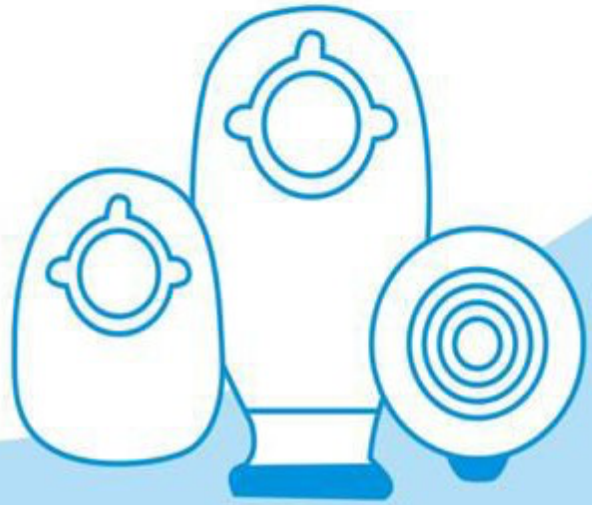

### Σάκος στομίας δύο τεμαχίων

1. Καθαρίστε με νερό το δέρμα γύρω από τη στομία.
2. Μια οπή έχει χαραχθεί ήδη στο άνοιγμα της βάσης και οι ασθενείς μπορούν να την ανοίξουν για να τοποθετήσουν τη βάση στο σημείο της στομίας.



3. Αφαιρέστε το προστατευτικό χαρτί από τη βάση.



4. Τοποθετήστε τη βάση, αφού την κόψετε καλά, στο σημείο της στομίας και πιέστε ελαφρώς με το δάχτυλό σας για να κολλήσετε τη βάση καλά. Σημείωση: τα δύο μικρά πτερύγια που περιβάλλουν την οπή και η ταινία πρέπει να είναι παράλληλα.



5. Φυσήξτε ελαφρώς στον σάκο πριν τον στερεώσετε για να μην κολλήσουν τα τοιχώματά του. Κρατήστε στη συνέχεια με τα δύο χέρια το εξωτερικό τμήμα στη βάση, από κάτω προς τα πάνω. Πιέστε με ένα δάχτυλο προσεκτικά το εξωτερικό τμήμα πάνω στη βάση για να κολλήσει καλά.



6. Όταν χρειάζεται να αλλάξετε τον σάκο, πιέστε με ένα δάχτυλο τη βάση και με το άλλο πιέστε το μικρό προεξέχον κομμάτι του εξωτερικού τμήματος και τραβήξτε για να αφαιρέσετε τον σάκο.



7. Όταν χρειάζεται να αλλάξετε τη βάση, με ένα δάχτυλο πιέστε το δέρμα και με ένα άλλο δάχτυλο τραβήξτε προσεκτικά τη βάση.



8. Χρησιμοποιήστε τον συνδετήρα για να στερεώσετε το άκρο του σάκου, γυρίστε 2 φορές και ενώστε την πόρπη πριν χρησιμοποιήσετε τον αναλώσιμο σάκο.



9. Ανοίξτε το άκρο του σάκου όταν αφαιρείτε τα κόπρανα, στρέψτε το άκρο του σάκου προς το ουροδοχείο και πλύνετε το άκρο του σάκου όπως στην εικόνα. Κλείστε προσεκτικά το άκρο του σάκου. Χρησιμοποιήστε μόνο μία φορά.



Σημείωση

1 Ο ασθενής μπορεί να χρησιμοποιήσει αυτό το προϊόν μόνο για κόπρανα.

2 Αυτή η βάση μπορεί να χρησιμοποιηθεί για 3-5 ημέρες σε κανονικές συνθήκες. Η παρατεταμένη χρήση ενδέχεται να προκαλέσει ερεθισμούς στο δέρμα.

3 Εάν ο σάκος είναι γεμάτος αέρα, αδειάστε τον αέρα χρησιμοποιώντας το άνοιγμα στο άνω άκρο του σάκου. Συνιστάται η χρήση φίλτρου ενεργού άνθρακα για την αντιμετώπιση της κακοσμίας.

4 Η βάση και ο σάκος μπορούν να χρησιμοποιηθούν μόνο μία φορά.



5 Η απόρριψη της βάσης και του σάκου δεν πρέπει να γίνεται στην τουαλέτα ή σε υπόνομο. Απορρίψτε υπεύθυνα, προστατέψτε το περιβάλλον



6 Βεβαιωθείτε ότι η κόλλα δεν προκαλεί δερματική αλλεργία.

Wuhan Sitaili Medical Apparatus Development Co., Ltd.
Room1-8,7th Floor,7th Building Guannan Fuxing Medical Industrial Park,No.62 Guanggu Road, East Lake New Technology Development Zone Wuhan City, Hubei Province, China, Tel：+86-27-82302765
EC Representative: Prolinx Gmbh
Address: Brehmstr.56,40239, Duesseldorf, Germany, Tel: 0049 211 3105 4698