STEADLIVE 思泰利
MEDICAL APPARATUS & HEALTHY NURSING

Ostomy Bag instruction

Two System

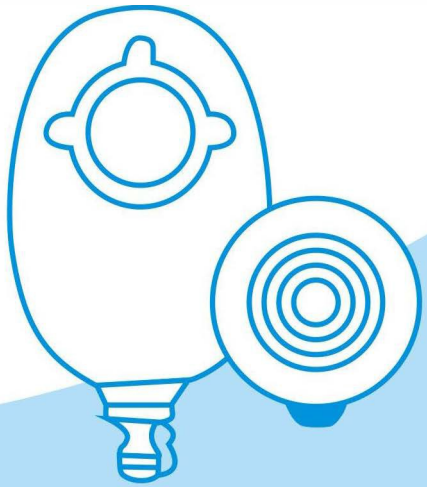

Two System○stomy Bag

1. Use the water to clean the skin around the stoma

2. A hole have been advanced open at the flange
the sufferers can cut a hole at the flange at the basis of the kind of stoma.



3. Close the valve which at the bottom of the ostomy bag.

9,

4. Remove the protection paper at the flange



5. Put the flange which have been cul well aimed at the stoma and stick onunclitly, press it down lightly by using the fi□'t-le the flange slick on well.
Notice: the two microtias which include the hole and sash at the parallel direction.



6. Blow a little air in to the bag before ftxrng Lh'o bag in order Lo prevenL the wall o(the pocket being sticked on .then hold the cutting sleeve aimed at the wedge seat using the two hands,from the bottom, the finger press it carefully along the cutting sleeve,make wedge seat and the cutting sleeve solidabsolutely.



7. When have to change the bag, put one finger lo press on flange, another finger to press the little protruding of the cutting sleeve and pull forth, unbolt the bag.



8. Use one finger to press the skin, another finger lo Lear out flange carefully when have lo change the flange.



Notice

1. The sufferer of the intestines open can use this productlto incept the ordure only.

2. The flange Lo mix this product can use 3–5 days in normal condiLion,iL can affect the effect of affixing if use delay,iL is not good Lo the skin .

3. The chassis and the bag which being exc- make hanged can noL be used again.



4. The flange and the bag which can not be washed in Lo the Loi let or cloaca, it can not be discareded at will, pay attention Lo the protection of the environment.



5. The skin uses Lo the gum allergy carefully.

Wuhan Sitaili Medical Apparatus Development Co., Ltd.
Room1-8,7th Floor,7th Building Guannan Fuxing Medical Industrial Park,No.62 Guanggu Road, East Lake New Technology Development Zone Wuhan City, Hubei Province, China.
Tel +86-27-82302765
EC Representative:Prolinx Gmbh
Address:Brehmstr.56,40239, Duesseldorf, Germany
Tel: 0049 211 3105 4698

STEADLIVE 思泰利
MEDICAL APPARATUS & HEALTHY NURSING

Οδηγίες χρήσης σάκων στομίας

Σάκος δύο τεμαχίων

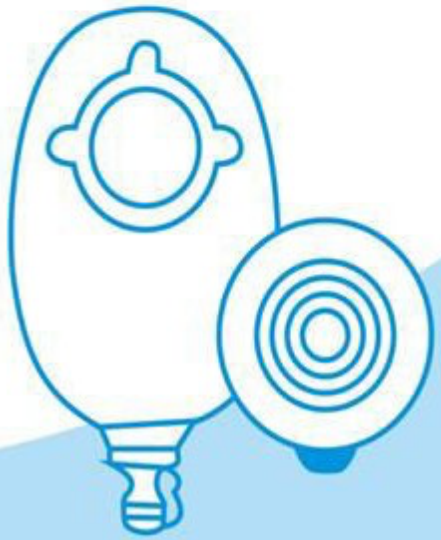

Σάκος στομίας δύο τεμαχίων

1. Καθαρίστε με νερό το δέρμα γύρω από τη στομία.
2. Μια οπή έχει χαραχθεί ήδη στο άνοιγμα της βάσης και οι ασθενείς μπορούν να την ανοίξουν για να τοποθετήσουν τη βάση στο σημείο της στομίας.



3. Κλείστε τη βαλβίδα στη βάση του σάκου στομίας.



4. Αφαιρέστε το προστατευτικό χαρτί από τη βάση.



5. Τοποθετήστε τη βάση, αφού την κόψετε καλά, στο σημείο της στομίας και πιέστε ελαφρώς με το δάχτυλό σας για να κολλήσετε τη βάση καλά.
   Σημείωση: τα δύο μικρά πτερύγια που περιβάλλουν την οπή και η ταινία πρέπει να είναι παράλληλα.



6. Φυσήξτε ελαφρώς στον σάκο πριν τον στερεώσετε για να μην κολλήσουν τα τοιχώματά του. Στη συνέχεια κρατήστε με δύο χέρια το εξωτερικό τμήμα πάνω στη βάση και πιέστε προσεκτικά από κάτω προς τα πάνω στη βάση για να κολλήσει καλά.



Wuhan Sitaili Medical Apparatus Development Co., Ltd.
Room1-8,7th Floor,7th Building Guannan Fuxing Medical Industrial Park,No.62 Guanggu Road, East Lake New Technology Development Zone Wuhan City, Hubei Province, China.
Tel：+86-27-82302765
EC Representative: Prolinx Gmbh
Address: Brehmstr.56,40239, Duesseldorf, Germany
Tel: 0049 211 3105 4698

7. Όταν χρειάζεται να αλλάξετε τον σάκο, πιέστε με ένα δάχτυλο τη βάση και με το άλλο πιέστε το μικρό προεξέχον κομμάτι του εξωτερικού τμήματος και τραβήξτε για να αφαιρέσετε τον σάκο.



8. Όταν χρειάζεται να αλλάξετε τη βάση, με ένα δάχτυλο πιέστε το δέρμα και με ένα άλλο δάχτυλο τραβήξτε προσεκτικά τη βάση.



Σημείωση

1. Ο ασθενής μπορεί να χρησιμοποιήσει αυτό το προϊόν μόνο για κόπρανα.
2. Αυτή η βάση μπορεί να χρησιμοποιηθεί για 3-5 ημέρες σε κανονικές συνθήκες. Η παρατεταμένη χρήση ενδέχεται να προκαλέσει ερεθισμούς στο δέρμα.
3. Η βάση και ο σάκος μπορούν να χρησιμοποιηθούν μόνο μία φορά.



4. Η απόρριψη της βάσης και του σάκου δεν πρέπει να γίνεται στην τουαλέτα ή σε υπόνομο. Απορρίψτε υπεύθυνα, προστατέψτε το περιβάλλον.



5. Βεβαιωθείτε ότι η κόλλα δεν προκαλεί δερματική αλλεργία.